

## Application Note # AN117

### Analysis of laced Drugs

The legal and illegal drugs comprise a wide range of different substances that differ strongly in their chemical and pharmacological characteristics. The number of available drugs in the market is constantly growing as new drugs are systematically synthesized with the intent to bypass the current narcotics laws. Most street drugs are not pure substances but mixtures that consist of two or more components. In order to maximize profits or to widen the spectrum of activity, drugs are laced with all kinds of substances or cut with other drugs.

As cutting agents usually substances are used that have chemical and physical properties similar to the drug itself. This prevents the detection of the contamination when the drug is for example solved or melted. The local anesthetic cocaine is being cut with other local anesthetics such as lidocaine or benzocaine in order to pretend higher cocaine content. Other often used cutting agents are milk sugar, pain relievers such as paracetamol, caffeine and the anti-parasitic agent levamisole that is normally used in veterinary medicine. Many drug deaths are directly linked to these cutting agents. Many serious side effects, including deaths, were reported from cocaine contaminated with levamisole. In practice it is often important to rapidly analyze such substance mixtures in order to supply medical aid or to expose criminal acts like the sale or smuggling of drugs.



Keywords	Instrumentation and Software
FT-IR	ALPHA-P
Laced drugs	OPUS 7.5
Mixture analysis	TICTAC ATR-FT-IR Drug Library
Identification	ATR-FT-IR Library Complete
Legal highs	



ALPHA FT-IR spectrometer with diamonds ATR module (ALPHA-P)

The ALPHA FTIR-Spectrometer is an ideal tool for the identification of pure and laced drugs. The analysis is based on infrared spectroscopy which is also called molecular spectroscopy. Infrared light induces vibrations of the molecules in the analyzed sample. The IR-light is therefore, depending on the sample characteristics, partly absorbed by the sample at specific wavelengths. The position and the intensity of the measured absorption peaks can be used for the identification of samples and mixtures. With the ALPHA, the measurement of the spectra is performed by using the Attenuated Total Reflection (ATR) technique. Thereby the sample needs to be simply pressed on a diamond crystal by using a pressure clamp. Apart from the homogenization of the sample there is no need for sample preparation, also no consumables or chemicals are required. Identification of the respective drug sample is being performed by an automatic search of the measured spectrum in spectral libraries. In the drug analyses shown in this application note, the spectrum search was performed by using the TICTAC-

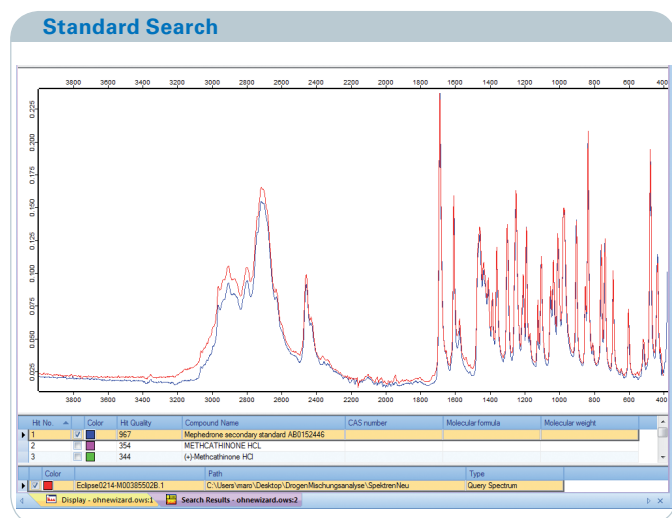


Figure 1: Spectra search of mephedrone. Red = measured spectrum, blue = library spectrum.

library that contains over 200 spectra of newest drugs and “legal highs” and the ATR-Complete library that contains over 26.000 spectra of a wide variety of substance classes. In combination with these libraries the ALPHA FT-IR-spectrometer is able to detect pure substances as well as mixtures of drugs. The standard search algorithm of the OPUS software is very powerful in finding the library spectrum matching best with the measured spectrum. Though, in cases of mixtures the measured spectrum might contain spectral contributions from several library spectra. To determine the different components present in such mixture spectra, OPUS offers a specialized algorithm for the analysis of mixtures. The mixture analysis determines within only a few seconds and fully automated the composition of a mixture.

### Example: The analysis of a pure drug.

The drug mephedrone is a former “legal high” and is forbidden in the EU since 2010. The spectrum shown in figure 1 was measured on a Platinum ATR-unit equipped ALPHA FTIR-spectrometer with diamond crystal (“ALPHA-P”). The spectra libraries were searched for a matching reference spectrum using the OPUS standard algorithm. When considering the very high similarity of the sample- and library-spectrum as well as the very high hit quality of 967 out of 1000 points it is obvious that the sample is most likely a pure substance. This is of course, as shown above, an exception since street drugs are very often contaminated as we are going to demonstrate in the next two examples.

### Example: Analysis of laced cocaine-hydrochloride

This example shows the analysis of cut cocaine-hydrochloride. Therefore a sample was measured with an ALPHA-P spectrometer and a measurement time of 25 seconds. The result of the mixture analysis is shown in figure 2. For the

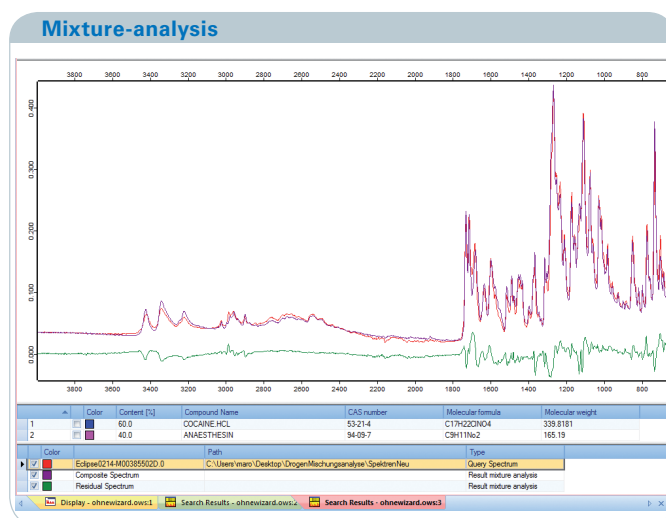


Figure 2: Mixture-analysis of laced cocaine-hydrochloride (red = measured spectrum, violet = composite, green = residual).

sake of clarity only the measured spectrum (red), the composite spectrum (calculated from the found single components, violet) and the residual spectrum (green) are shown. The residual spectrum shows the differences between the calculated composite spectrum and the measured spectrum. The more even and flat the residual spectrum is, the better the match between the calculated composite spectrum and the measured spectrum. In our example we have a nearly perfect match between the composite spectrum and the measured spectrum, thus the peaks of the residual spectrum are of only limited intensity. Besides the main component cocaine-HCl the local anestheticum anaestheticum (benzocaine) was found. The given percentage points

describe the spectral contribution of the single components to the overall spectrum. Figure 3 shows the measured and the composite spectrum together with the spectra of the single components in detail.

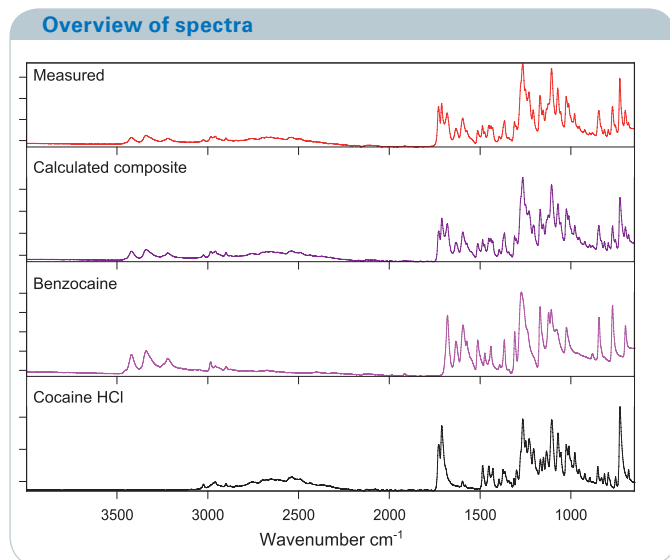


Figure 3: From top: Measured spectrum, composite spectrum, component benzocaine, component cocaine HCl.

**Example:  
Analysis of “crack”.**

Crack is being made from cocaine salt (usually cocaine-hydrochloride) by heating it together with sodium bicarbonate (baking soda). Thereby, amongst others, the free cocaine base is formed. In contrast to cocaine-hydrochloride it can be smoked because of its lower melting point. Crack is usually laced too and is only rarely available as a pure product. Figure 4 shows the mixture analysis of a real street sample that was also measured with the ALPHA-P. It is obvious from the mixture analysis result, that the sample

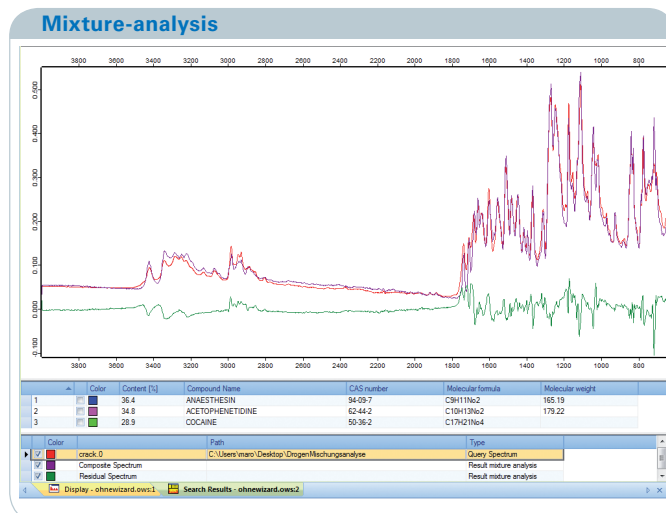


Figure 4: Mixture-analysis of laced crack (red = measured spectrum, violet = composite, green = residual).

is also laced with the local anesthetic anaesthesia. Additionally there is also a considerable amount of the pain reliever acetophenidine (phenacetine) detectable. Acetophenidine acts as a mild mood enhancer and is, due to its renal toxicity, forbidden in most countries. Due to its similar physical properties it is, however a widely used cutting agent and is used sometimes in very high concentrations.

**Summary**

The ALPHA FTIR-spectrometer allows analyzing drugs and drug mixtures in a fast and comfortable manner. The combination of the dedicated drug library TICTAC and the very broad ranging “ATR-Complete”-library allows to identify drugs, legal highs, unusual cutting agents as well as such substances that only appear to be a drug.



**Bruker Optics Inc.**

Billerica, MA · USA  
Phone +1 (978) 439-9899  
Fax +1 (978) 663-9177  
info@brukeroptics.com

**Bruker Optik GmbH**

Ettlingen · Deutschland  
Phone +49 (7243) 504-2000  
Fax +49 (7243) 504-2050  
info@brukeroptics.de

**Bruker Hong Kong Ltd.**

Hong Kong  
Phone +852 2796-6100  
Fax +852 2796-6109  
hk@brukeroptics.com.hk

[www.bruker.com/optics](http://www.bruker.com/optics)